

Private: L-Kynurenine ELISA kit – Research – Former

Ref: BA-E-2200R-Former

The L-Kynurenine ELISA is an easy-to-use assay tailored for the quantification of Kynurenine across large series of samples. Intended for research use only, the KYN ELISA features a lower limit of detection at 45.7ng/ml and a minimal sample volume of 20µl, thus allowing longitudinal studies in mice.

Sample type Plasma, serum, cell culture supernatant

Capacity 96 tests

Sensitivity < 45.7ng/ml

Range 100 - 10000ng/ml

Assay time Sample acylation 90 min, ELISA overnight

Reactivity Reacts with all species

References [> 30 citations in literature](#)

INFORMATIONS

Product overview

Product name	L-Kynurenine ELISA kit
Description	Enzyme immunoassay (ELISA) for the quantitative determination of L-Kynurenine in biological fluids and cell supernatant. For research use only
Format	96-well plate
Samples	Plasma, serum, cell culture supernatant
Minimal sample volume	20µL
Reactivity	Reacts with all species
Standard range	0/100 – 10000ng/ml
Sensitivity	< 47.5ng/ml
Specificity	No significant cross-reactivity was observed with L-Kynurenine analogs such as L-Tryptophan, 3-Hydroxy-DL-Kynurenine, 5-Hydroxy-DL-Tryptophan, Tyrosine, Serotonin, Phenylalanin, L-Asparagine and Kynurenic acid
Assay time	Sample acylation 90 min and ELISA overnight
Storage	Store at 2-8°C for to 6 months
Datasheets	Instructions for use , Material Safety Datasheet

The kit for in-vitro-diagnostic (IVD) use can be ordered with the catalog no. [BA E-2200](#).

PROTOCOLS

Sample collection & storage

Plasma/Serum: Do not use lipemic, haemolytic samples, as well as samples containing precipitates or fibrin strands. Store samples at 2-8°C for up to 48h or -20°C for longer period (up to 6 months)

Sample preparation

Sample acylation (90 min)

ELISA

L-Kynurenine antiserum overnight incubation, revelation and read steps (1h)

Detailed protocol

[Download instructions for use](#)


REFERENCES

Product citation

Product pictures




L-Kynurenine ELISA kit

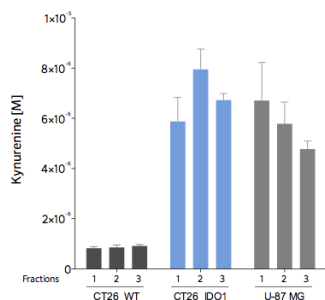

Determination of L-Kynurenine levels in cell cultures through microdialysis collection and by ELISA quantification

Murine CT26 colorectal cancer cell line WT or stably transfected with vector containing cDNA encoding for indoleamine 2,3 dioxygenase (IDO1) or Human U-87 MG glioblastoma cell line were cultured for 48 hours. Cell culture was subjected to microdialysis collection (3 fractions collected) and kynurenine was measured using the Kynurenine ELISA kit (BA-E-2200). As expected, kynurenine level was higher in IDO1-proficient CT26 cells than in parental (WT) CT26 cell lines, and also high in U87-MG cells.



L-Kynurenine quantification by ELISA in 20µl mice plasma samples

Determination of L-Kynurenine levels in cell cultures through microdialysis collection and by ELISA quantification

Kynurenine ELISA cross-validation by GC/MS in human plasma samples


L-Kynurenine quantification by ELISA in 20µl mice plasma samples

Determination of L-Kynurenine levels in CT26 cell cultures by ELISA

Kynurenine ELISA - typical standard curve

L-Kynurenine quantification by ELISA in 20µl mice plasma samples

C57BL/6 mice were challenged intraperitoneally with 10mg/kg of LPS or with its vehicle (PBS). Twenty four hours after LPS exposure, animals were bled at the tail vein using EDTA-Monovette®. Kynurenine was quantified by mean of the Kynurenine ELISA kit. As demonstrated in literature (Bessede et al. Nature, 2014), LPS challenge induces a substantial increase in kynurenine plasmatic level.



Kynurenine ELISA cross-validation by GC/MS in human plasma samples

Determination of L-Kynurenine levels in cell cultures through microdialysis collection and by ELISA quantification

Kynurenine ELISA cross-validation by GC/MS in human plasma samples


L-Kynurenine quantification by ELISA in 20µl mice plasma samples

Determination of L-Kynurenine levels in CT26 cell cultures by ELISA

Kynurenine ELISA - typical standard curve

Kynurenine ELISA cross-validation by GC/MS in human plasma samples

Citrate-anticoagulated human plasma samples were processed for Kynurenine measurement by gas-chromatography/mass-spectrometry and ELISA. As shown here, ELISA and GC/MS-based results showed a high correlation.

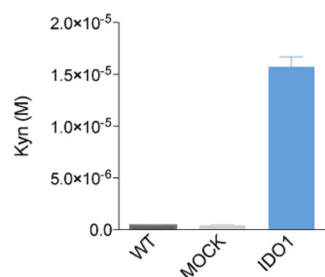

Determination of L-Kynurenine levels in CT26 cell cultures by ELISA
Determination of L-Kynurenine levels in cell cultures through microdialysis collection and by ELISA quantification
Kynurenine ELISA cross-validation by GC/MS in human plasma samples
L-Kynurenine quantification by ELISA in 20µl mice plasma samples
Determination of L-Kynurenine levels in CT26 cell cultures by ELISA
Kynurenine ELISA - typical standard curve
Determination of L-Kynurenine levels in CT26 cell cultures by ELISA


Murine CT26 colorectal cancer cell line was stably transfected with either empty vector (Mock) or vector containing cDNA encoding for indoleamine 2,3 dioxygenase (IDO1). Cells were cultured for 48 hours and kynurenine was measured using the Kynurenine ELISA kit. As expected, kynurenine level was higher in IDO1-proficient CT26 cells than in mock or parental (WT) CT26 cell lines.



L-Kynurenine ELISA kit



L-Kynurenine ELISA kit



Kynurenine ELISA - typical standard curve
Determination of L-Kynurenine levels in cell cultures through microdialysis collection and by ELISA quantification
Kynurenine ELISA cross-validation by GC/MS in human plasma samples
L-Kynurenine quantification by ELISA in 20µl mice plasma samples
Determination of L-Kynurenine levels in CT26 cell cultures by ELISA
Kynurenine ELISA - typical standard curve
Kynurenine ELISA - typical standard curve

Example of standard curve obtained with the Kynurenine ELISA Kit. In this competitive ELISA, optical density is inversely correlated with Kynurenine levels. Only serves as example - do not use for calculation.

Contact information

Immusmol

229 Cours de l'Argonne

33 000 Bordeaux - France

Tel: +33 (0) 5 6431 1170

www.immusmol.com

To order, review, ask for technical support, visit product page at:

https://www.immusmol.com/?post_type=product&p=867